

A Simple Pressure Sensor Signal Conditioning Circuit

INTRODUCTION

A simple signal conditioning circuit should allow the output of the amplifier to be independent of the sensor used, providing interchangeability and high level output at very low cost. A laser trimmed resistor on the sensor's compensation board programs the gain of an external amplifier to normalize the pressure sensitivity variation.

SIMPLE SIGNAL CONDITIONING CIRCUIT

The signal conditioning circuit shown in Figure 1 provides a precision constant current source for sensor excitation and an instrumentation amplifier with the gain programmed by sensor feedback resistor r .

For a detailed discussion of the compensation circuit, and for output voltages other than 0-5V, please refer to Application Notes TN-001 and APP-103 to APP-105.

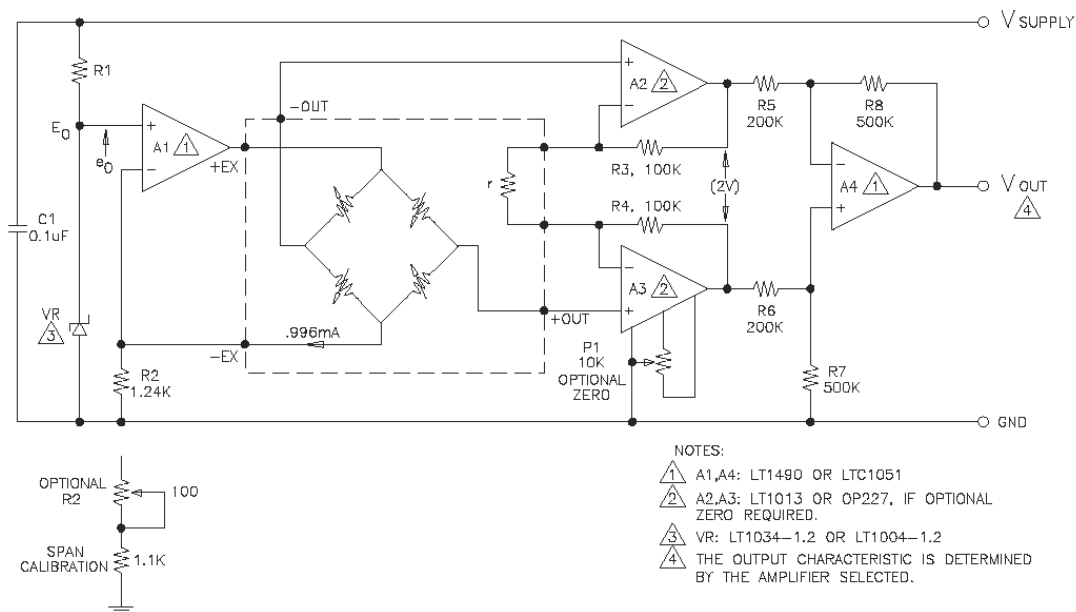


Figure 1 - Basic Signal Conditioning Circuit

A Simple Pressure Sensor Signal Conditioning Circuit

CIRCUIT DETAILS

The current source is controlled by the $\pm 1\%$ band-gap reference diode, VR. The reference current IO is defined by:

$$I_o = (E_o - e_o)/R_2 \quad [1]$$

Where: E_o - diode reference voltage: 1.235V $\pm 1\%$ (LT1034-1.2 or LT1004-1.2)

e_o - offset of amplifier A1 (~ 0)

R2 - current set resistor

Selecting amplifier A1 with an offset voltage below 1 mV and a $\pm 1\%$ tolerance of resistor R2 delivers current $I_o = 0.996$ mA with typical accuracy of $\pm 1.4\%$.

The differential input stage of the instrumentation amplifier, A -A has a gain of $\text{Gain} = 1 + (R + R)/r$.

The gain set resistor r is trimmed for R3=R4=100K and a differential output voltage of 2V.

OPTIONAL ZERO ADJUST

If the optional zero adjustment is required, use OP227 amplifiers instead of the LT1013 and add the zeroing potentiometer P1.

The zero range is typically ± 4 mV referenced to the input with a differential offset below 0.5 mV. This leaves about a ± 3.5 mV zeroing range for the compensation of the sensor offset which is typically below ± 1 mV.

OUTPUT

The output stage of the instrumentation amplifier provides additional amplification R8/R5 and translates the differential floating voltage from the first stage into a single ended output voltage. The equation for the overall output voltage is:

$$V_{out} = 2 \cdot A \cdot R_8 / R_5 = 5.000V @ A = 1 \quad [3]$$

A is the Ratio between the actual excitation current IO and the specified current.

A Simple Pressure Sensor Signal Conditioning Circuit

ACCURACY AND CALIBRATION

The overall accuracy of the span is effected by the accuracy of feedback resistors R_1 through R_4 . Using $\pm 1\%$ resistors such as Mepco/Electra 5063Z, the typical gain error will be about $\pm 0.24\%$. The accuracy error may be decreased when matched thin film resistors are used such as Beckman 694-3-A. The combined span error of the entire signal conditioning circuit at a reference temperature will then typically be about 1.1% without any adjustment or pressure testing. This will be superimposed on the sensor's accuracy of $\pm 1\%$.

OPTIONAL SPAN CALIBRATION

If additional calibration and normalization is desired, resistor R_2 can be replaced with a series combination of a potentiometer and a resistor (Figure 1). The potentiometer can be adjusted to set the bridge excitation current (I) to achieve the exact span voltage (S) with full scale pressure applied to the sensor.

GAIN ERROR

If no pressure source is available, the gain error of the amplifier can be reduced by using the procedure outlined below. This method may be used instead of using the precision resistors discussed above for R_2 through R_8 . The sensor span error of $\pm 1\%$ will remain, however. Calibration procedure:

- replace resistor r with an external resistor $7.50\text{ K} \pm 0.1\%$
- check gain K of the instrumentation amplifier and calculate the gain ratio X (in reference to the idea that gain $K_0 = 69.028\text{V/V}$), where $X = K / K_0$
- set current $I_0 = 0.996/X(\text{mA})$ by adjusting the potentiometer, thus completing calibration.

Assuming a $6.4\text{ k}\Omega$ (50°C) maximum bridge resistance, a 0.996 mA bridge current and a 1.2V diode reference voltage, it follows that the maximum output voltage of amplifier A1 can approach 7.4V . Also, the positive saturation voltage at 1 mA out-put current for the LTC1051 amplifier is 0.5V . Therefore, the minimum excitation voltage which is a function of the current source and amplifiers used would be 7.9V ($7.4\text{V} + 0.5\text{V}$) for the LTC1051. For the LT1490, the minimum excitation voltage should be 7.6V . The maximum excitation voltage is limited by the voltage handling characteristics of the specific amplifier used.

A Simple Pressure Sensor Signal Conditioning Circuit

OUTPUT SPAN S_O VARIATION

Resistor r is laser trimmed for each unit using the following equation:

$$r = \frac{2R_F}{\frac{V_{amp}}{S_i} - 1} \quad [4]$$

Where: S_i = sensor span value (V) at a reference excitation current ($I_o = 0.996$ mA).

r = resistance in (k)

$R_F = 100$ K feedback resistor

V_{amp} = amplified output

The output span S_o at the differential output of amplifiers A3- A2 (see Figure 1) for any other feedback resistor R in K is given by:

$$S_O = AS \left(\frac{r+2R}{r} \right) = 2A \left[\frac{R}{100} + S_i \left(\frac{100-R}{200} \right) \right] \quad [5]$$

Where: $A = I / I_o$, ratio of excitation current I to reference current I_o .

If 100 k feedback resistors are used, the expression for output span is simplified to:

$$S_c = 2A \quad [6]$$

and is constant for all sensors independent of sensor span S_i . The output span is also independent of the pressure range of the sensor. For other values of the feedback resistors (R), the output span (S_o) will vary with the sensor span (S_i). Assuming $I = I_o$, we can calculate S_o variations.

Table 1. Output Span (S_o) Variation

R	$S_O(S_i=40$ mV)	$S_O(S_i=90$ mV)	S_O variation [$\pm\%$]
50 K	1.0200	1.0450	1.23
75 K	1.5100	1.5225	0.41
99 K	1.9804	1.9809	0.01
100 K	2.0000	2.0000	0.00
101 K	2.0196	2.0191	0.01
200 K	3.9600	3.9100	0.63
500 K	9.8400	9.6400	1.0

A Simple Pressure Sensor Signal Conditioning Circuit

As seen in Table 1, a large deviation from the optimum feedback resistance of 100 k is tolerable while maintaining transducer interchangeability. For the optimum feedback resistance (100 k), calibration accuracy is a function of the accuracy of the excitation current, feedback resistors and sensor trimming. The inaccuracy caused by the excitation current and feedback resistors can be made negligible by the use of precision components. Therefore without pressure testing, a 1% system accuracy can be achieved. The standard gain programming resistor r has a TCR ± 50 ppm/ $^{\circ}$ C and a trimming range of 2.5 to 12.5 k. For volume orders, a custom trimming algorithm can be made to achieve any desired output span.

ORDERING INFORMATION

NORTH AMERICA

Measurement Specialties
45738 Northport Loop West
Fremont, CA 94538
Tel: 1-800-767-1888
Fax: 1-510-498-1578
Sales: pfg.cs.amer@meas-spec.com

EUROPE

Measurement Specialties
(Europe), Ltd.
26 Rue des Dames
78340 Les Clayes-sous-Bois, France
Tel: +33 (0) 130 79 33 00
Fax: +33 (0) 134 81 03 59
Sales: pfg.cs.emea@meas-spec.com

ASIA

Measurement Specialties
(China), Ltd.
No. 26 Langshan Road
Shenzhen High-Tech Park (North)
Nanshan District, Shenzhen 518107
China
Tel: +86 755 3330 5088
Fax: +86 755 3330 5099
Sales: pfg.cs.asia@meas-spec.com

The information in this sheet has been carefully reviewed and is believed to be accurate; however, no responsibility is assumed for inaccuracies. Furthermore, this information does not convey to the purchaser of such devices any license under the patent rights to the manufacturer. Measurement Specialties, Inc. reserves the right to make changes without further notice to any product herein. Measurement Specialties, Inc. makes no warranty, representation or guarantee regarding the suitability of its product for any particular purpose, nor does Measurement Specialties, Inc. assume any liability arising out of the application or use of any product or circuit and specifically disclaims any and all liability, including without limitation consequential or incidental damages. Typical parameters can and do vary in different applications. All operating parameters must be validated for each customer application by customer's technical experts. Measurement Specialties, Inc. does not convey any license under its patent rights nor the rights of others.